

Sgarlato
Silastic System

SHIP / Shaw




Sgarlato Silastic System

SHIP / Shaw


Time tested for over 25 years

The Sgarlato Lesser Toe implants are spacers and stabilizers made of medical-grade silicone elastomer used in hammertoe correction. The arthroplasty implant method helps restore alignment and motion by preserving the joint space relationship, maintaining toe length integrity, and providing sagittal and transverse plane stability¹.

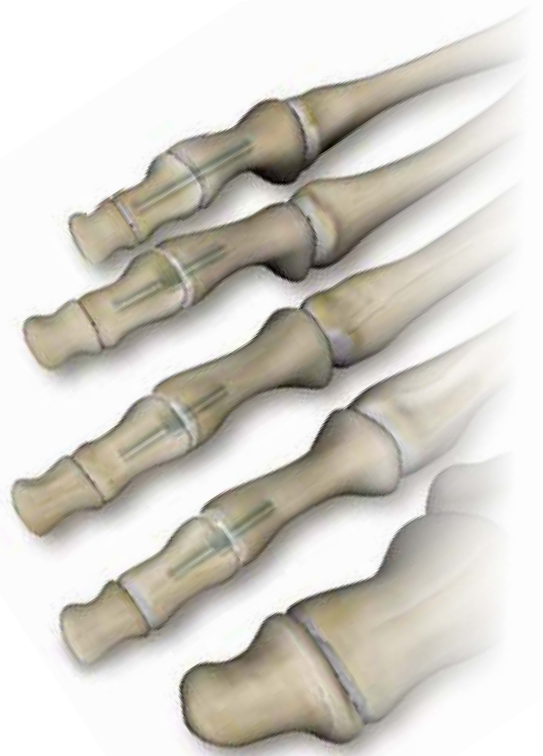

92% Reported patient satisfaction rate²

Less than 1% Reported removal rate with Sgarlato Design Implant²

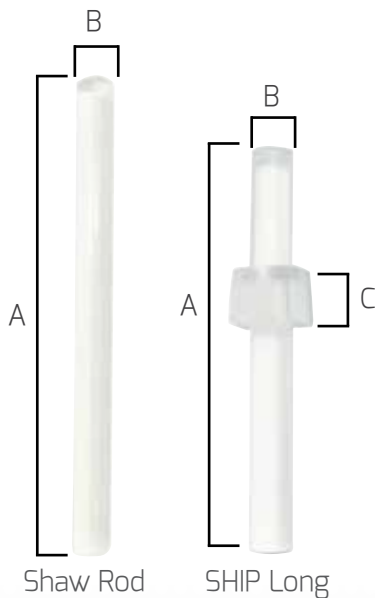

IMPLANT ORDERING

Description	A	B	C
SHIP Long Flexible	21.5mm	2.0mm	3.0mm
SHIP Long Regular	21.5mm	2.3mm	3.0mm
SHIP Long Stiff	21.5mm	2.5mm	3.0mm
Shaw Rod Flexible	26mm	2.0mm	-
Shaw Rod Regular	26mm	2.3mm	-
Shaw Rod Stiff	26mm	2.5mm	-

1. Sgarlato, T. E., Carine, T. A., Andrews, M. C. Sutter lesser toe implant. J. A. P. M. A. 78:335, 1988.
2. Sgarlato TE, Tafuri S: Digital Implant Arthroplasty: Clinics in Podiatry Medicine and Surgery 13(2):255-62, May 1996

FUSION ORTHOPEDICS, LLC.

4135 S. Power Rd. Suite 110
Mesa, Arizona 85212 USA
(800)-403-6876
Sales@fusionorthopedics.com



FDA Cleared

All Rights Reserved. Sgarlato is a Trademark of Fusion Orthopedics, LLC. D-4360-SLSX-1 Rev A

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Fusion Orthopedics does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate the breadth of Fusion's product offerings. A surgeon must always refer to the package insert, product label and / or instructions for use before using any Fusion Orthopedics product.